

Qualitätskontrollzertifikat / Quality Control Certificate

Kitcharge / Lot

EQ0134

IFU-Version

138-16

03.07.2025

Verw. bis / Exp.

2027-04-30

!New!

Prüfdatum /

Date of control



Verwendete Reagenzien / Reagents used	Lot	Standard	Standard Kurve / Standard curve
Teststreifen / Antigen coated strips	ECQ0175	Ref.- Werte / Ref. Values	Parameter A 0,049
Standardserum / Standard serum	ECQ0194	OD 0,88	B 1,289
Negativ Kontrolle / Negative control	ECQ0168		C 4,047
Konjugat / Conjugate	KJQ089+++	Units 37,2 U/ml	D 2,329
Quantifizierungsgrenzen / Limits of quantification		U/ml 5 - 500	
Grenzwertbereich / Borderline range		U/ml 10 - 15	

OD Bereich / OD Range 405 nm, Standardserum / Standard serum										
0,44 - 0,49	0,50 - 0,54	0,55 - 0,60	0,61 - 0,65	0,66 - 0,71	0,72 - 0,76	0,77 - 0,82	0,83 - 0,87	0,88	U/ml	Interpretation
< 0,14	< 0,16	< 0,18	< 0,19	< 0,21	< 0,23	< 0,24	< 0,26	< 0,27	< 10,0	neg
0,14 - 0,20	0,16 - 0,23	0,18 - 0,25	0,19 - 0,28	0,21 - 0,30	0,23 - 0,33	0,24 - 0,35	0,26 - 0,38	0,27 - 0,39	10,0 - 15,0	gw / borderline
> 0,20	> 0,23	> 0,25	> 0,28	> 0,30	> 0,33	> 0,35	> 0,38	> 0,39	> 15,0	pos

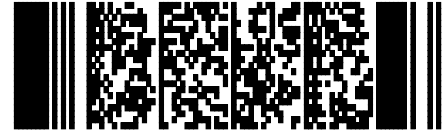
OD Bereich / OD Range 405 nm, Standardserum / Standard serum										
U/ml	0,88	0,89 - 0,96	0,97 - 1,03	1,04 - 1,11	1,12 - 1,19	1,20 - 1,27	1,28 - 1,34	1,35 - 1,42	1,43 - 1,50	Interpretation
< 10,0	< 0,27	< 0,28	< 0,31	< 0,33	< 0,35	< 0,38	< 0,40	< 0,43	< 0,45	neg
10,0 - 15,0	0,27 - 0,39	0,28 - 0,41	0,31 - 0,44	0,33 - 0,48	0,35 - 0,51	0,38 - 0,55	0,40 - 0,58	0,43 - 0,61	0,45 - 0,65	gw / borderline
> 15,0	> 0,39	> 0,41	> 0,44	> 0,48	> 0,51	> 0,55	> 0,58	> 0,61	> 0,65	pos

Formeln für spezielle Auswertesysteme
Special case formulas

OD = 0,447 x MV(STD) entspricht oberem cut-off/ corresponds to upper cut-off
OD = 0,303 x MV(STD) entspricht unterem cut-off/ corresponds to lower cut-off
Concentration= exp(4,047-ln(2,28/(MV(Sample) x0,88/ MV(STD)-0,049)-1)/1,289)

15
10

Institut Virion\Serion GmbH
Friedrich-Bergius-Ring 19
D-97076 Würzburg

**Zusätzliche Barcodes mit Formeln für / Additional Barcodes with formulas for
Revelation™ DSX / DS-Matrix™****4PS- Formel / 4PS-formula**
$$\exp(4.047 - \ln(2.280 / (\text{Sample} * 0.880 / S - 0.049) - 1) / 1.289)$$
**Gültigkeitsbereich / Validity Range**
$$0.440 \leq S1 \leq 1.496$$
**If OD Sample < Parameter A**
$$\text{if } Ti < (0.049 * (S1 / 0.880)) \text{ then } Ti = (0.049 + 0.001) * (S1 / 0.880)$$
**If OD Sample > Parameter D**
$$\text{if } Ti > (2.329 * (S1 / 0.880)) \text{ then } Ti = (2.329 - 0.001) * (S1 / 0.880)$$
**If OD Negative control < Parameter A**
$$\text{if } NC1 < (0.049 * (S1 / 0.880)) \text{ then } NCi = (0.049 + 0.001) * (S1 / 0.880)$$
